





27-inch Full HD IPS Surgical Monitor


| 27HK510S |

Optimal Image Quality for Fine Surgery

Full HD* IPS Display with sRGB 115%

The Full HD IPS display with sRGB 115% is designed to fit with other Full HD surgical devices. It enables surgeons to view accurate, realistic images by maximizing compatibility and clearer, brighter color reproduction, especially in the red color spectrum.

*Full HD: 1920x1080



DICOM* Part 14 I Brightness Stabilization

The LG Surgical Monitor carefully measures and sets every grayscale tone as well to create a monitor compliant with DICOM Part 14 and ensure the most accurate outcome. In addition, sensors measure backlight brightness and automatically compensate for fluctuations in brightness caused by ambient temperature and aging for a consistently stable display.

*DICOM: Digital Imaging and Communications in Medicine.




Designed for Use in the Operating Room

IP35 (Front) & IP32 (Except for Front): Dustproof & Water Resistant

To ensure protection against contact with substances such as blood or bodily fluids, LG Surgical Monitors are cleanable and durable, with ratings of IP35 on the front and IP32 on the rest, securing them from any direction.



Water Resistance




Anti-reflection I Anti-fingerprint

The LG Surgical Display with anti-reflection screen reduces glare so your surgical display is easier to see in challenging and changing indoor lighting conditions. Also, its anti-fingerprint screen provides resistance to the appearance and attachment of fingerprints and smudges.

Long-lasting Eye Comfort


Flicker Safe

Flicker Safe reduces the onscreen flicker level to almost zero, which helps minimize eye strain and eye fatigue. By combining Flicker Safe with the proven picture quality of IPS technology, users can comfortably work throughout the day.

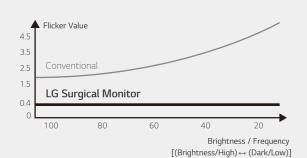



Specification

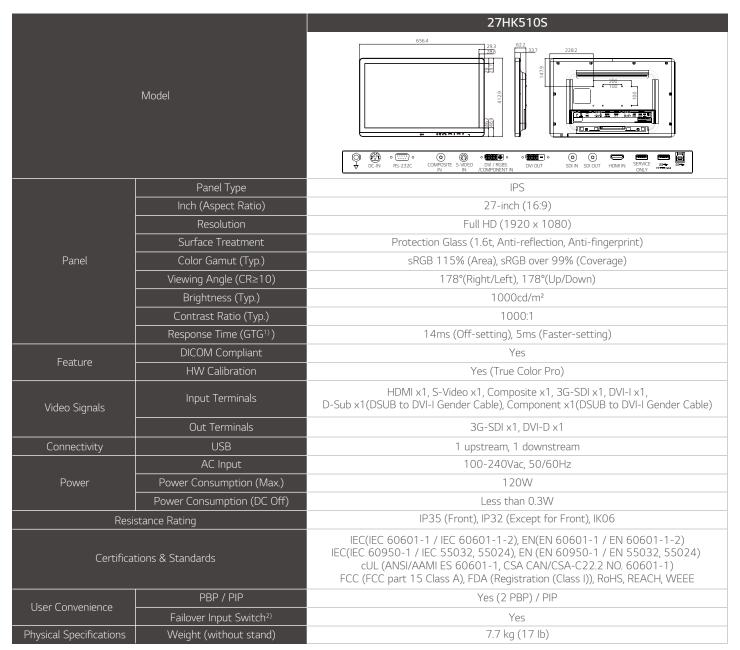

¹⁾ GTG : Gray to gray response time



LG Electronics Inc.

http://www.lge.com/global/business

²⁾ Failover Input Switch will be available from May 22, 2020.

^{*}The monitor stand is not included with the surgical monitor.